


robert scheers


pioneer
5090

Notes:

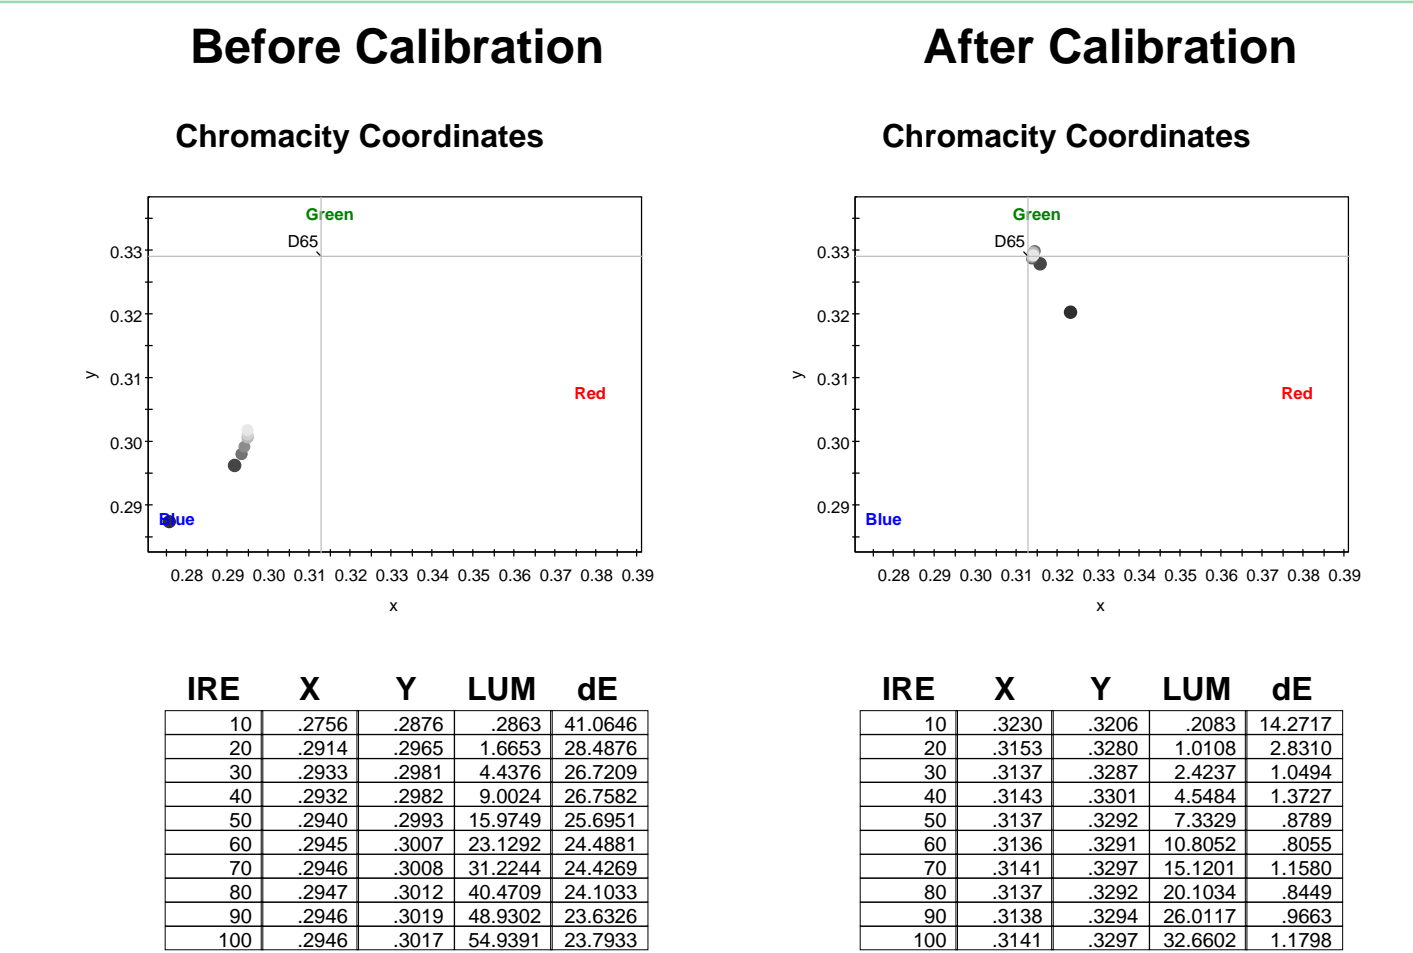

Before Calibration


Temperature Tracking

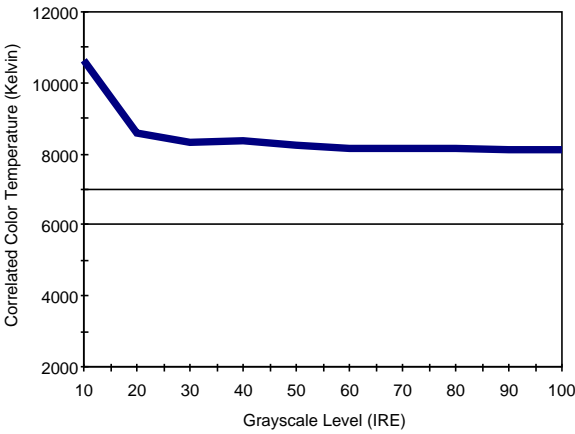

IRE	TEMP
10	10.635
20	8.560
30	8.337
40	8.352
50	8.248
60	8.160
70	8.157
80	8.137
90	8.120
100	8.129

After Calibration


Temperature Tracking

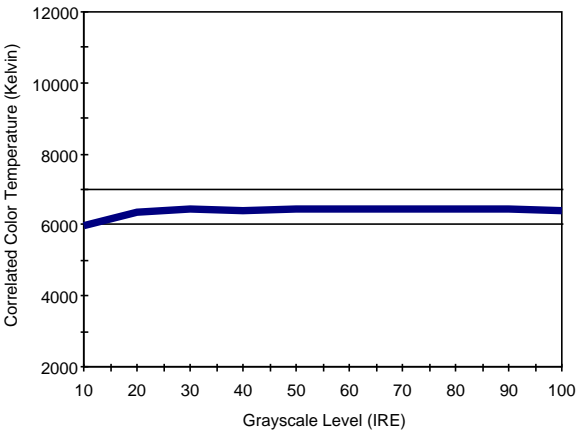

IRE	TEMP
10	5.989
20	6.372
30	6.452
40	6.411
50	6.448
60	6.454
70	6.425
80	6.449
90	6.439
100	6.423

Before Calibration


Color Tracking

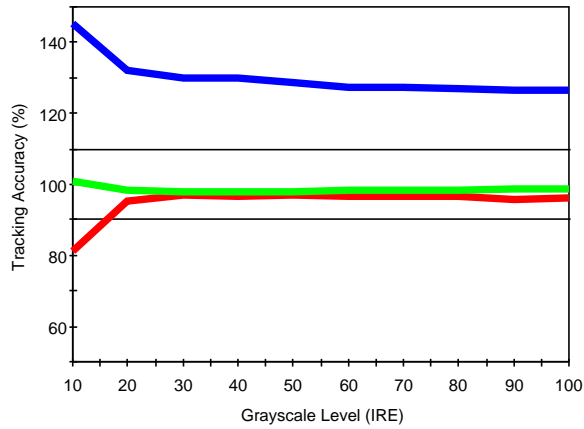

IRE	R	G	B
10	1.2340	.9896	.6875
20	1.0473	1.0193	.7576
30	1.0328	1.0212	.7696
40	1.0355	1.0205	.7693
50	1.0327	1.0200	.7768
60	1.0355	1.0177	.7854
70	1.0358	1.0175	.7858
80	1.0374	1.0167	.7881
90	1.0425	1.0147	.7916
100	1.0415	1.0151	.7905

After Calibration

Color Tracking

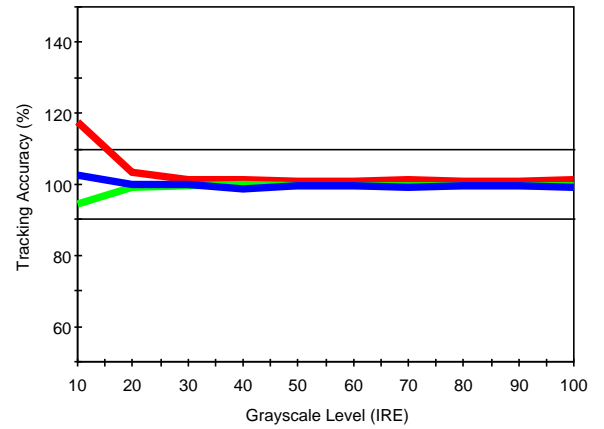

IRE	R	G	B
10	.8518	1.0577	.9733
20	.9657	1.0106	1.0006
30	.9870	1.0039	1.0008
40	.9889	1.0021	1.0122
50	.9897	1.0027	1.0041
60	.9904	1.0026	1.0032
70	.9890	1.0024	1.0090
80	.9902	1.0025	1.0042
90	.9894	1.0026	1.0059
100	.9888	1.0025	1.0091